

Weightron Bilanciai Ltd,
Titan Works
Bridge Way off Broombank Road,
Chesterfield Trading Estate,
Chesterfield S41 9QJ, UK
Tel: 01246 260062
Fax: 01246 260844
www.weightron.com



Weightron Bilanciai Ltd,
Unit 4b, Block 4
Westpark, Chelston
Wellington TA21 9AD, UK
Tel: 01823 662355
Fax: 01823 662017
www.weightron.com



CALIBRATION CERTIFICATE

This Calibration Certificate is issued in accordance with the UKWF Code of Practice for the calibration of Non Automatic Weighing Machines. All weights used are traceable to NPL

Customer

*P A Moody
Nest Rd
Galeshead
NE10 8YA
LOCATION*

Machine Details

Cust ref	
Make	<i>Bilanciai</i>
Model	<i>DD700</i>
Ser No	<i>T16000498</i>
Capacity	<i>50 1000 kg</i>
e/d	<i>120 kg</i>
Working cap	

Test Weights

Set No.	Cert No.	Date Cal
<i>FB1-19</i>	<i>9787</i>	<i>Oct 22</i>
<i>FB po-104</i>	<i>9787</i>	<i>Oct 22</i>

Cert Interval	<i>12M</i>
Next Cert	<i>Sept 24</i>

Tolerance +/-	kg
<i>0-10000</i>	<i>20</i>
<i>10000-40000</i>	<i>40</i>
<i>40000-50000</i>	<i>60</i>

Comments
FLT - 4820
Wagon - 20720


<i>3</i>	<i>4</i>	<i>6</i>	<i>8</i>
<i>1</i>	<i>5</i>	<i>5</i>	<i>7</i>

X

AS FOUND LINEARITY & HYSTERESIS

Load	Loading	Dev	Unloading	Dev
<i>0</i>	<i>0</i>	<i>0</i>	<i>0</i>	<i>0</i>
<i>2000</i>	<i>2000</i>	<i>0</i>	<i>2000</i>	<i>0</i>
<i>6000</i>	<i>6000</i>	<i>0</i>	<i>6000</i>	<i>0</i>
<i>12000</i>	<i>12000</i>	<i>0</i>	<i>12000</i>	<i>0</i>
<i>18000</i>	<i>18000</i>	<i>0</i>	<i>18000</i>	<i>0</i>
<i>20720</i>	<i>20720</i>	<i>0</i>	<i>20720</i>	<i>0</i>
<i>30720</i>	<i>30720</i>	<i>0</i>	<i>30720</i>	<i>0</i>
<i>38720</i>	<i>38720</i>	<i>0</i>	<i>38720</i>	<i>0</i>
<i>43540</i>	<i>43540</i>	<i>0</i>	<i>43540</i>	<i>0</i>


DEFINITIVE LINEARITY & HYSTERESIS

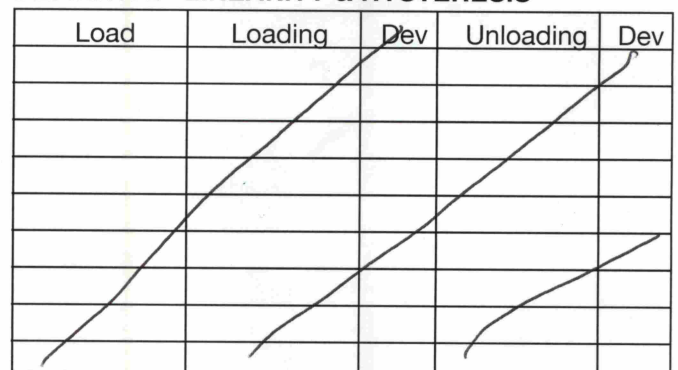

Repeatability

Load	Ind	Ind	Ind
<i>43540</i>	<i>43540</i>	<i>43560</i>	<i>—</i>


Repeatability

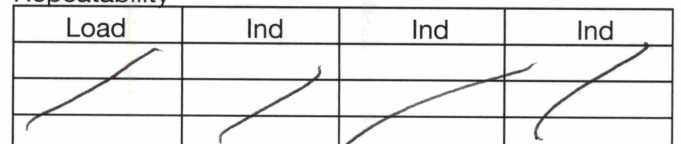

Eccentric Load

Reading	Dev	Reading	Dev
<i>1 6820</i>	<i>0</i>	<i>2 6820</i>	<i>0</i>
<i>3 6800</i>	<i>-20</i>	<i>4 6820</i>	<i>0</i>
<i>5 6800</i>	<i>-20</i>	<i>6 6820</i>	<i>0</i>
<i>7 6820</i>	<i>0</i>	<i>8 6800</i>	<i>-20</i>

Eccentric Load

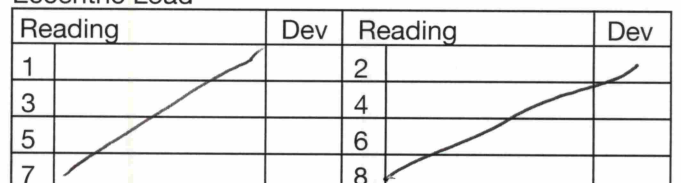

Signature *Bill* Name *IAN DILLON* Date *28-9-23*